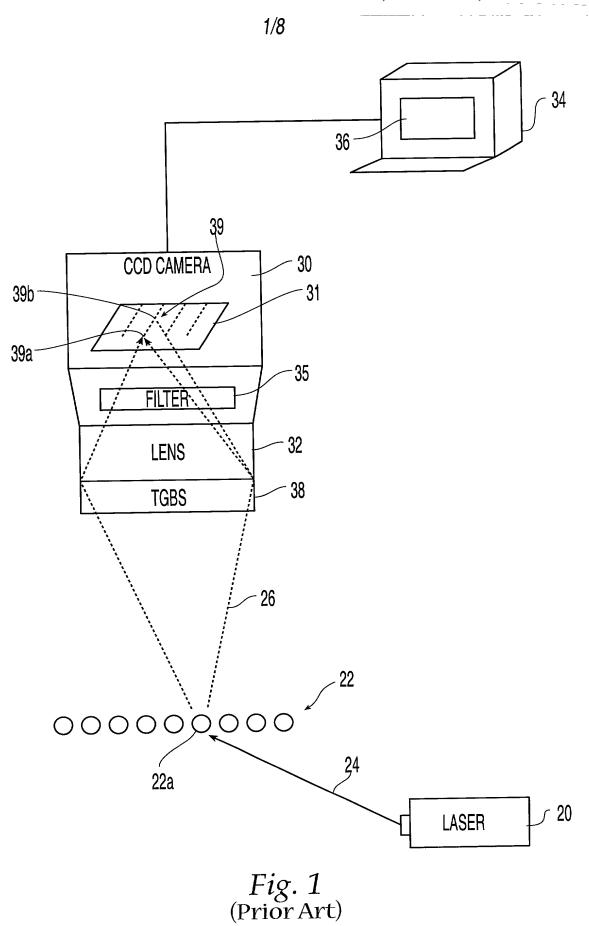
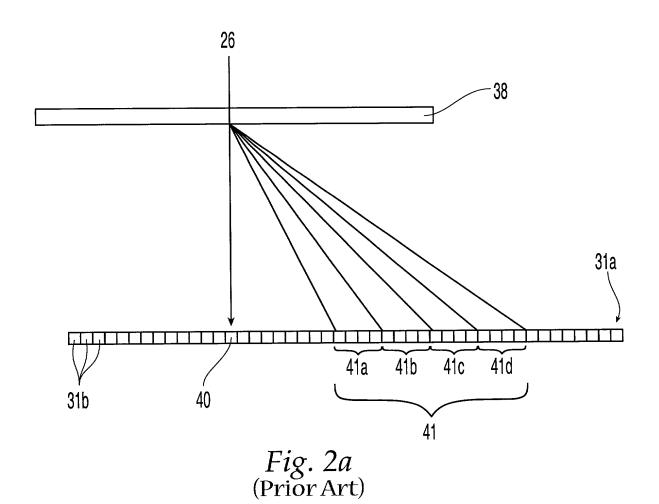
Appl Of: McVey et al.; Appl No. 09/849,239; Filed: 5/7/01; For: Electrophoretic Method and System Having Internal Standards For Color Calibration; Group: 2185; Atty Dkt # 9046-050; Tel: 202-496-4400; Sht lof8









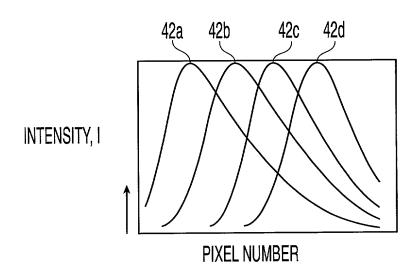


Fig. 2b (Prior Art)






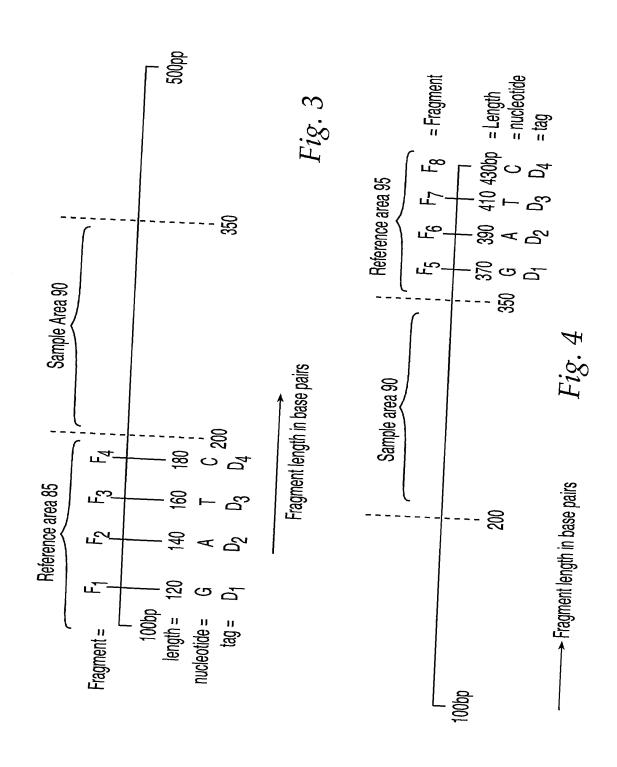


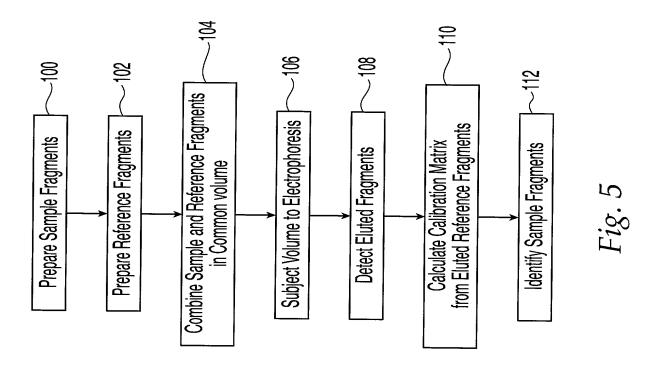




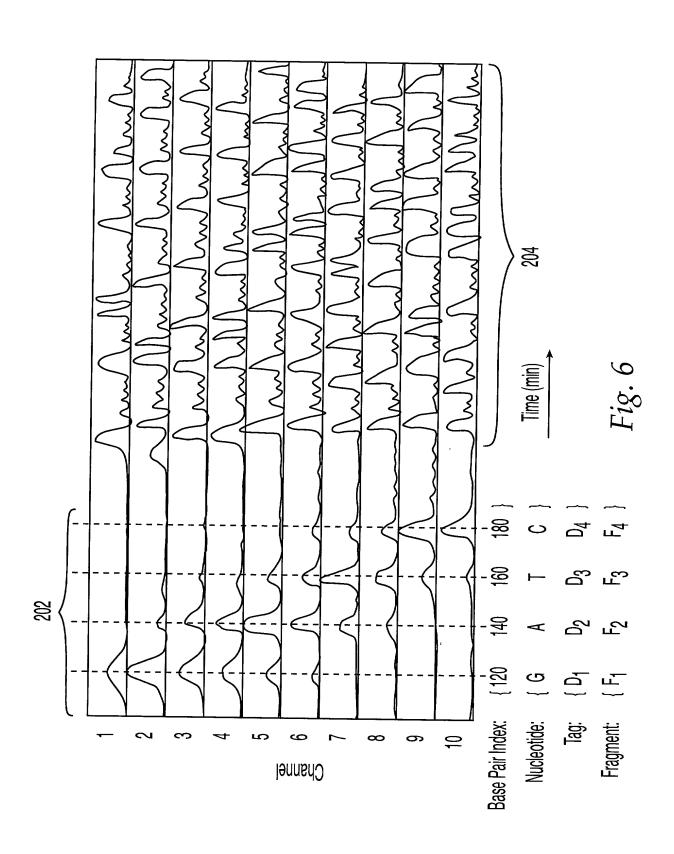



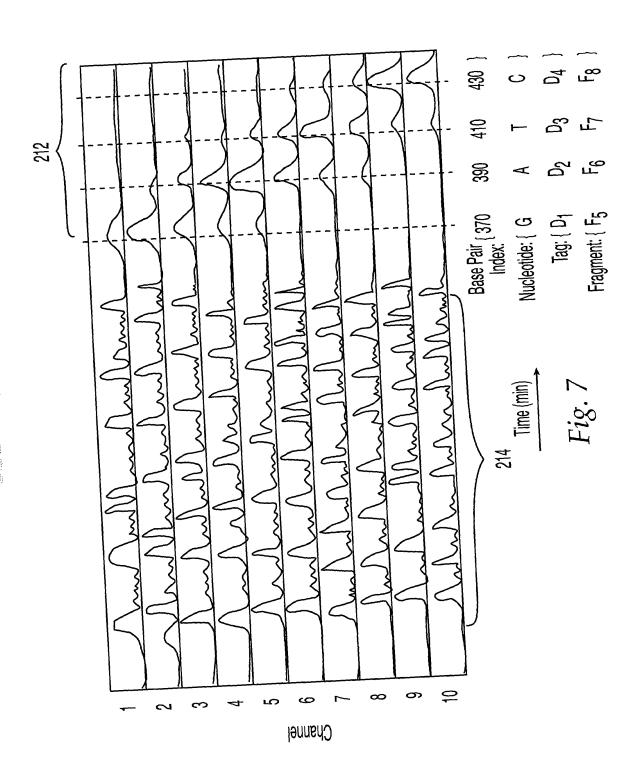

Appl Of: McVey et al.; Appl No. 09/849,239; Filed: 5/7/01; For: Electrophoretic Method and System Having Internal Standards For Color Calibration; Group: 2185; Atty Dkt # 9046-050; Tel: 202-496-4400; Sht 7 of 9

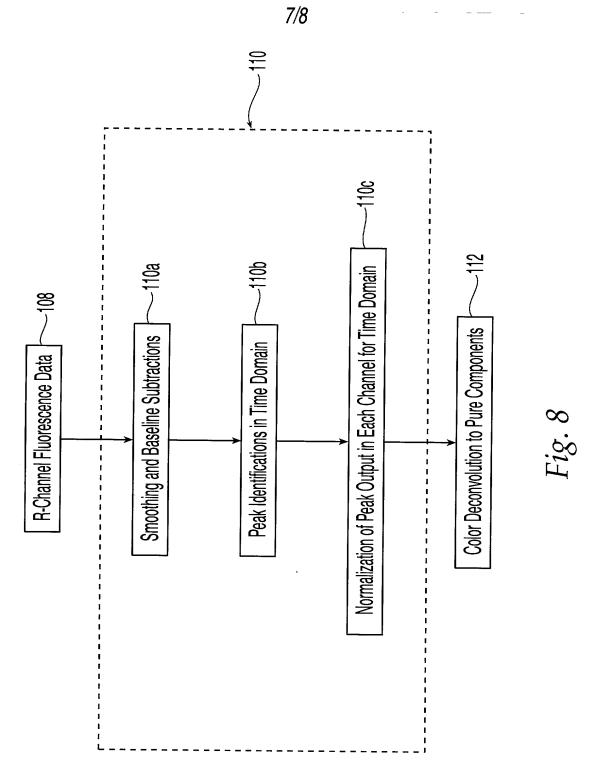

Calibration Coefficients for each base

		G	Α	T	C
Channel Number	1 2 3 4 5 6 7 8 9	.408 1 .887 .566 .394 .265 .152 .091 .059	.037 .205 .722 1 .721 .428 .287 .202 .120 .069	.021 .034 .063 .244 .754 1 .691 .403 .274	.016 .021 .023 .027 .067 .359 .925 1 .604

Fig. 9